



アルカリ性条件(pH9.5)下の連続分析

Continuous analysis under basic pH condition


SunShell C18 2.6 μm, 50 x 2.1 mm i.d.

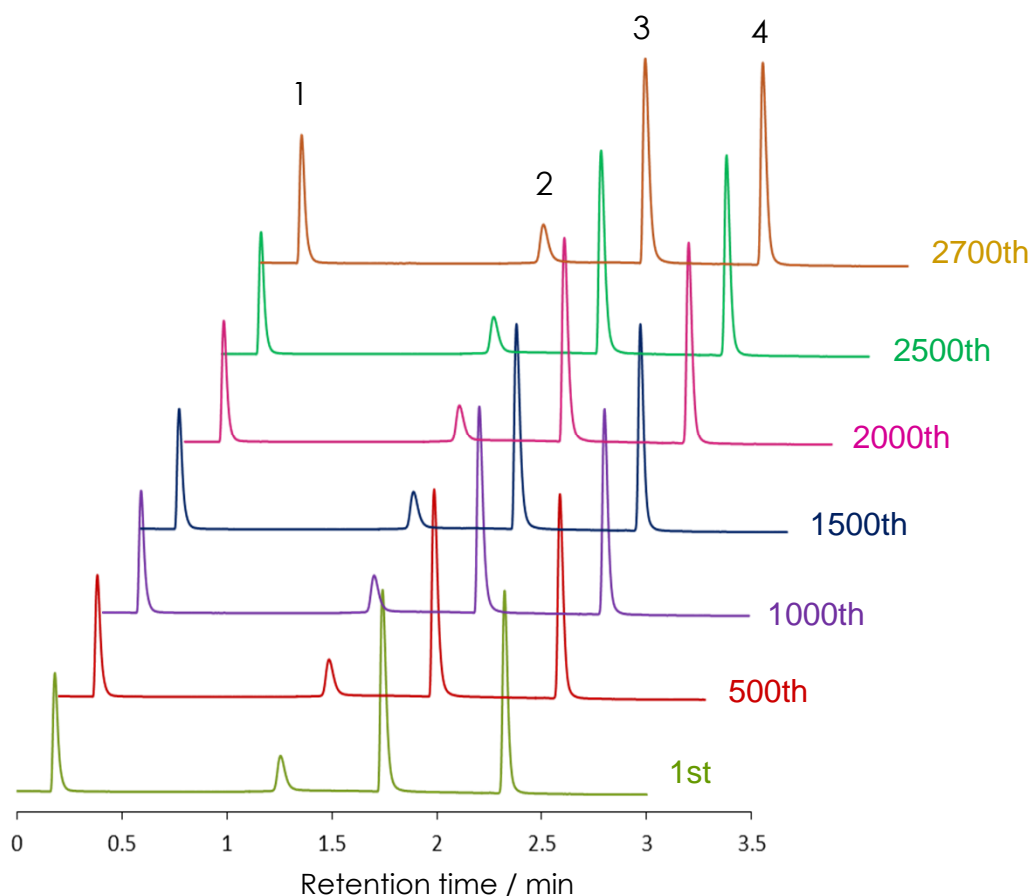


1. Uracil




2. Propranolol



3. Nortriptyline



4. Amitriptyline



Column: SunShell C18, 2.6 μm 50 x 2.1 mm
Mobile phase: A) 10 mM Ammonium bicarbonate pH 9.5
B) Acetonitrile

Gradient program:

Time (min)	0	1	3	3.1	5
% B	30	90	90	30	30

Flow rate: 0.5 mL/min
Temperature: 40 °C
Detection: UV@250nm
Injection volume: 0.5 μL
Sample: 1=Uracil, 2=Propranolol,
3= Nortriptyline, 4=Amitriptyline

Instrument
Hitachi Chromaster®
Detector: 5410
Oven: 5310
AutoSampler: 5260
Pump: 5160

